

Technical Definition

Lap Joint Shear test
Carbon Fiber Composite

You shall respect the HSE policy of your laboratory for each performed test.

Instructions to participant laboratories

Please read carefully these instructions BEFORE starting the tests.


- Five specimens (225 x 50 x 3,0 mm) are supplied to each participant – 5 results must be provided.
If one result is missing, your test will be considered as an outlier. A RCA shall be completed.
- The specimens have to be dried during 48 hours (0/+10) at 70°C (+/- 3), kept in controlled conditions and tested within the next 8 hours after the drying.
- All tests have to be performed at room temperature in accordance with the requirements of **AITM 1-0065 issue 2** (see note below).


The tests shall be performed respecting the following conditions:

- One operator only
- One testing machine only
- Tests performed in sequence

Note: All specimens should be tested applying hysteresis loop as described in **AITM 1.0065 Issue 2, paragraph 8.3.1** (first specimen requirement should be avoided). Load values for hysteresis loop have been calculated as function of failure load determined in Homogeneity tests.

- Predicted Failure load: **15000 N (To be confirmed later)**
- Initial Loop Point (B): **5000 N**
- Final Loop Point (C): **1500 N**

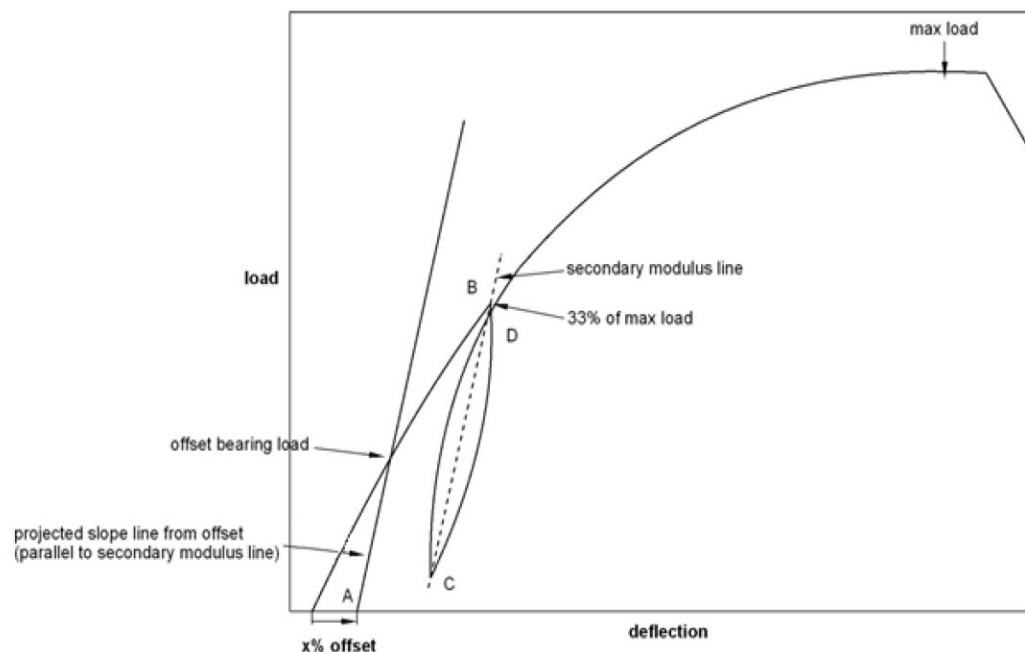

| | | |
|---|-------------|---|
| Revision No. 1 | Page 2 of 3 | Technical Definition Lap Joint Shear test Carbon Fiber Composite |
|  | | |
| Kit Lap Joint Shear PTP 2020 | | |

Additional information concerning the fasteners will be communicated later.

4. The following information need to be reported:

| Characteristic | Unit | Significant digits | Mandatory / Not mandatory | Evaluated Yes/no |
|---|------|--------------------|---------------------------|------------------|
| Specimen length | mm | X,XX | Mandatory | No |
| Specimen thickness | mm | X,XX | Mandatory | No |
| Specimen width | mm | X,XX | Mandatory | No |
| Strain System (Extensometer, LVDT, etc) | N/A | N/A | Mandatory | No |
| Offset bearing load | N | XXX | Mandatory | Yes |
| Maximum load | N | XXX | Mandatory | Yes |
| Failure load | N | XXX | Mandatory | Yes |
| Failure mode | N/A | N/A | Mandatory | No |
| Upload of the official test report | N/A | N/A | Mandatory | No |

All evaluated characteristics will be analysed according to the algorithm A and S (ISO 13528 – 2015) and evaluated using z-score.

5. Testing shall start **as soon as test specimens are received**. Please contact the following e-mail address for any technical or administrative query.

| | |
|---|--|
| Submission date : | July 15th, 2020 |
| Technical and administrative support : | info@ptpscheme.com |

6. Instructions for submission of results are detailed on the website:

<https://ptpscheme.com/>

7. To ensure the confidential treatment of your results in the final report, you will be allocated a unique identity number when you register for the program.
8. Collusion and falsification of your PTP results are totally forbidden. In case of identification or suspicion of collusion or falsification, the laboratory will be excluded from the program and the sponsors will be immediately informed. The sponsors could ask you proofs of your records and analyses, so be sure to conserve data, curves and specimens.
9. The tested specimens do not need to be sent back to PTP.



Technical Definition

Lap Joint Shear test
Carbon Fiber Composite

APPENDIX : Instructions for IRR participation

The Internal Round Robin participation (IRR) is **optional** and **independent** from your PTP participation.

Confidentiality : The IRR results and reports are confidential and only accessible by your laboratory. They are not shared with the scheme sponsors or any other accreditation or certification bodies.

The extra samples shall be tested according to the following table:

| | Operator 1 | Operator 2 | Operator 3 | Operator 4 | Operator X |
|-----------------------|---------------------|------------|------------|------------|------------|
| Test machine 1 | PTP kit (5 samples) | 3 samples | 3 samples | 3 samples | 3 samples |
| Test machine 2 | 3 samples | | | | |
| Test machine 3 | 3 samples | | | | |
| Test machine Y | 3 samples | | | | |

Operator 1 (OP1) is to be the most experienced operator currently conducting tests on a regular basis and shall perform tests on all machines (TM1, TM2, TM3...)

Test Machine 1 (TM 1) is to be the most utilised machine for this test in your laboratory and shall be tested by all operators (OP1, OP2, OP3...)

Example: A laboratory has 2 operators and 3 test machines. They receive a PTP kit and 9 extra specimens.

Operator 1 shall test the PTP kit on TM1, 3 specimens on TM2 and 3 specimens on TM3.

Operator 2 shall test 3 specimens on TM1.

The IRR results have to be submitted on a separate results form available on the PTP website.

The identification of operators and test machines you provide will appear on the IRR final report.

These identifications will not be seen by other laboratories.

The IRR results will be classified against the acceptance classes of the kit Lap Joint Shear-2020.

Reminder: Laboratories are not permitted to switch specimens between the PTP kit and IRR samples. The traceability of the samples will be checked during the evaluation. Laboratories found to have switched samples will invalidate their PTP participation.

REVISION HISTORY

| Issue Date | Issue N° | Changes |
|------------|----------|-------------------|
| 05/03/2020 | 1 | Document creation |